

## Differential Pulse Voltammetry: Evolution of an In Vivo Methodology and New Chemical Entries, A Short Review

Francesco Crespi<sup>1,\*</sup>

<sup>1</sup>Voltammetry Lab, Medicine Research Centre, Verona, Italy

### Background

In 1924 Heyrovsky found that current at a mercury electrode was not directly proportional to the applied voltage, but there was presence of an extra-current determined by the oxidisable chemicals present in the solution. Such extra current, that is proportional to the concentration of the compound(s) oxidized and/or reduced, is called polarographic current when obtained at a mercury electrode, is called voltammetric current when obtained at all other types of electrodes [1, 2].

Different types of voltammetric techniques are available the most common of which are chrono-amperometry linear voltammetry, cyclic voltammetry, and pulse voltammetry [3,5].

These methodologies are mainly based on the application of a "dynamic" oxidation or oxido-reduction [ox - red] potential and the resulting analysis of electrons "freed" by the chemical(s) under analysis (see Figure 1).

### Technique

Voltammetric measurements are taken with a three-electrode potentiostat system made of a silver/silver chloride (Ag/AgCl) reference electrode, a copper or silver wire auxiliary (counter) electrode both approximately 100  $\mu\text{m}$  in diameter and a working electrode (see Figure 2). Nowadays, the working electrode is mainly a carbon fiber micro electrode (figure 1).

### Electrodes for Voltammetry

Different types of voltammetric electrodes have been developed since 1969, the most performing type appear to be the carbon based electrodes and in particular the carbon fiber - micro electrode ( $\mu\text{CFE}$ ) (see Figure 3) [3,5,6].

The association of voltammetry with these electrodes become an electrochemical methodology allowing continuous, in real time and in situ detection of oxidizable chemicals.

The turning point of the use of these

**Corresponding author:** Francesco Crespi, Voltammetry Lab, Medicine Research Centre, Verona, Italy, Email: [fm.crespi@libero.it](mailto:fm.crespi@libero.it)

**Keywords:** vivo methodology, voltammetric techniques

**Received:** Apr 01, 2020

**Accepted:** Apr 21, 2020

**Published:** Apr 28, 2020

**Editor:** Zhe-Sheng Chenz, Professor, Department of Pharmaceutical Sciences, College of Pharmacy and Allied Health Professions, St. John's University, United States.

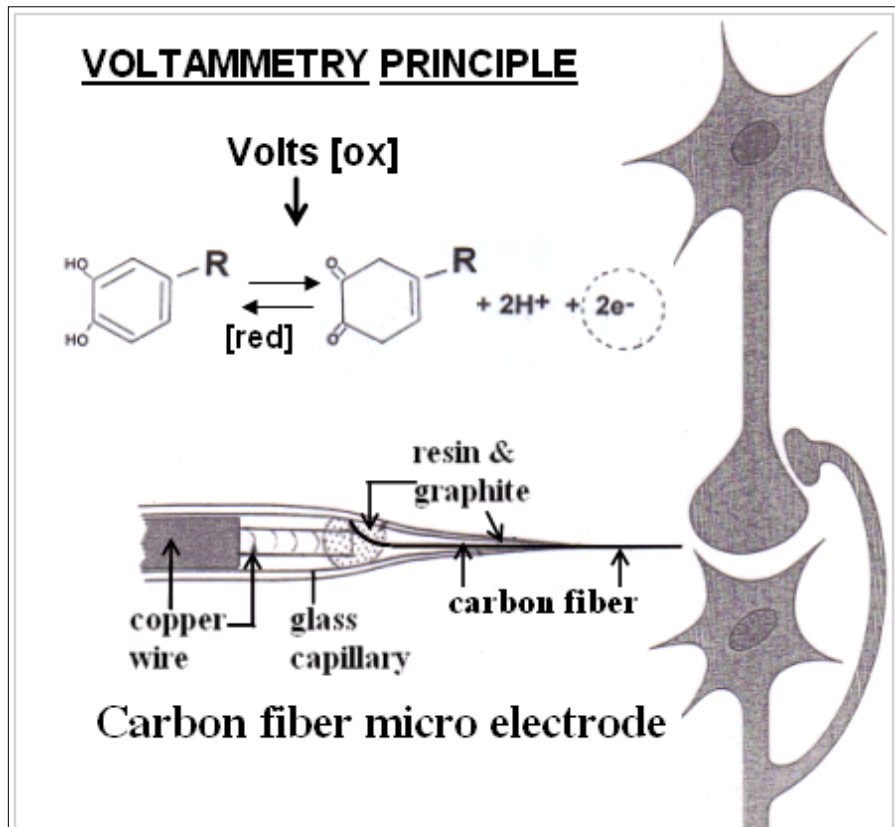


Figure 1. voltammetry principle and schematic representation of the carbon fiber micro electrode (modified from ref 5 with permission).

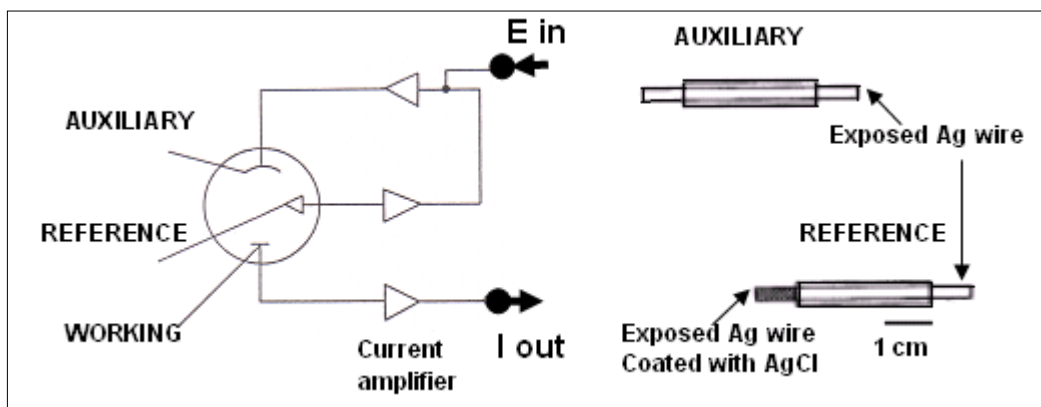


Figure 2. schematic representation of the three-electrode potential system [left] and the reference and auxiliary electrodes (modified from ref 6 with permission).

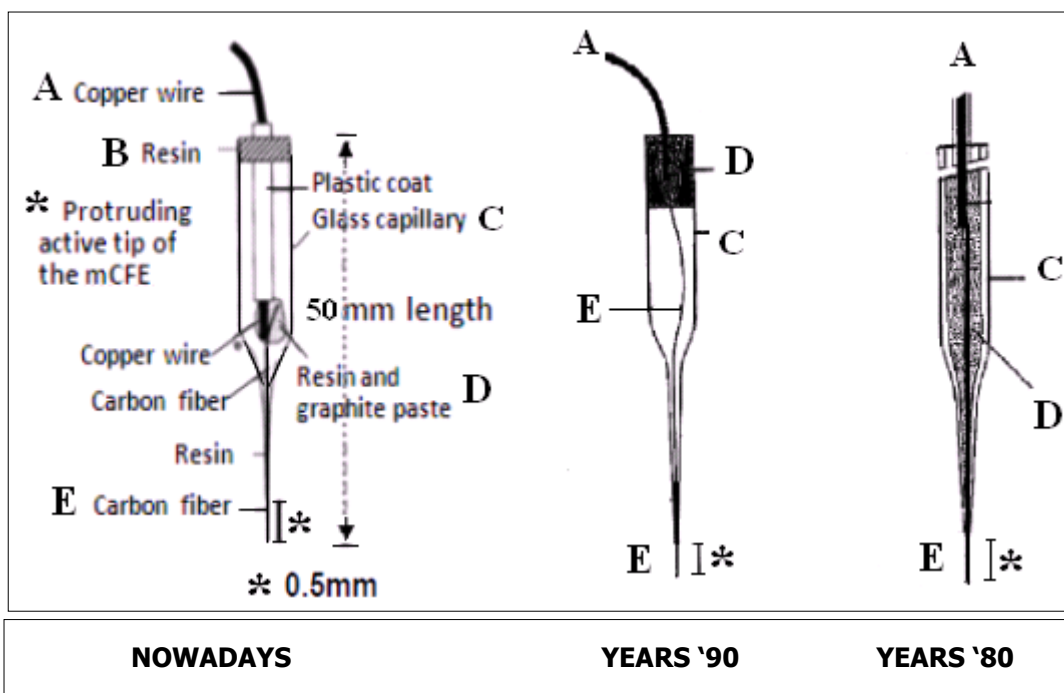


Figure 3. schematic representation of the evolution upon time of the manufacture of the carbon fiber micro electrode used as working electrode for voltammetry. A: is the conductive wire, B: resin alone or D: mixed with graphite paste. E is the carbon fiber that can vary between 6, 7, 10, 30  $\mu\text{m}$  diameter. \* is the protruding tip of the carbon fiber from the glass capillary (C). The length of the tip can vary from 0.1mm up to 1- 2mm in function of the size of the brain area monitored or the biological tissue analyzed, i.e. aortic(11), gastric tissue (12) (modified from ref 5 with permission).

micro-sensors has been the application of a variety of electrical pre-treatments that are applied to the sensors before use. This has indeed improved drastically sensitivity and selectivity for analysis of electro-active chemicals and this in particular when the electrochemical methods of normal pulse as well as differential pulse voltammetry are employed [7 – 10]. Then, evolutions on pre-treatment of the  $\mu\text{CFE}$  have also been proposed. In particular, in addition to the electrical pre-treatment, a chemical pre-treatment consists in coating the protruding active tip of the micro sensor with Nafion (Sigma). Nafion is a sulphonated polymer repelling acids while attracting bases as it is negatively charged. This electrode is then called Nafion  $\mu\text{CFE}$  and it allows selective detection of dopamine and serotonin in vitro as well as in vivo with a greater sensitivity for the latter [13]. Further development of such chemical pre-treatment is the coating with a mixture of Nafion and Crown ether

(Sigma). The reresulting sensor is called NaCro  $\mu\text{CFE}$  and shows an improved sensitivity for the selective detection of these amines [14] and in particular that of dopamine [15].

#### Differential Pulse Voltammetry (DPV)

DPV combines aspects of chronoamperometry and linear sweep voltammetry and exhibits high selectivity and sensitivity. Small voltage pulses of a constant amplitude (20-50 mV) are superimposed 3-5 times per second upon a linear voltage ramp (see Figure 4). The current is sampled immediately before ( $i_A$ ) a pulse and subtracted from the current at the end of the pulse ( $i_B$ ), then the difference  $i_B - i_A$  is expressed in terms of potential. This consents to DPV to combines the main advantage of chronoamperometry (suppression of charging current) with the resolution of sweep voltammetry, as it performs a local differentiation of the voltammogram obtained by linear voltammetry. The

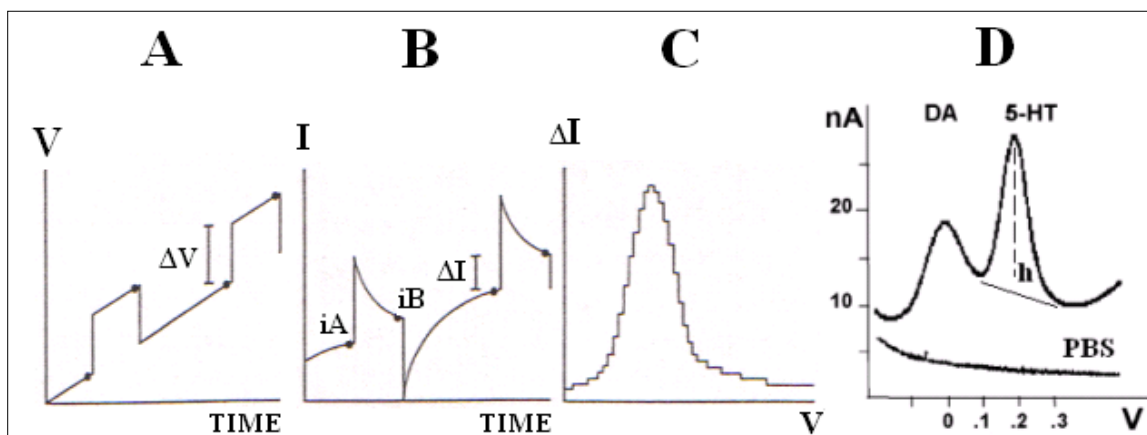


Figure 4. In Differential pulse voltammetry the applied potential is A: a linearly increasing ramp upon which small pulses of amplitude  $\Delta V$  are superimposed. B: two measurements are made for each pulse; one just before the pulse [ $i_A$ ] and one just before the end of the single pulse [ $i_B$ ], to yield the differential current value  $\Delta I$ . C: the differential current  $\Delta I$  is reported against the applied potential  $V$  to give the peak-shaped voltammogram (peak). D: in vivo, i.e. in rat striatum, DPV monitoring the peaks of dopamine [DA] and serotonin [5-HT] at approximately 10mV and 200mV, respectively [h: size of the peak in nanoAmperes [nA].

overlap between two oxidisable compounds is eliminated providing that they oxidize at sufficiently distinct potentials (at least 50-100 mV between both). Thus, the oxidation of a compound produces a sharp peak rather than the broad peak or plateau of linear sweep voltammetry, resulting in higher resolution [16].

The association of DPV with pre-treated  $\mu$ CFE appears to be the best methodology for rapid in situ analysis of electro-active compounds. No other combination of electrode and voltammetric method allows the same sensitivity with high resolution between oxidizable chemicals and in particular:

**i) in vitro**, with the active tip of the sensor immersed in buffered solution [7, 17, 3];

**ii) ex vivo**, with the active tip of the sensing electrode in contact with several tissue such as brain slices [18,19], the endothelium of rat aortic rings for detection of nitric oxide and nitrites [11, 20, 21] or in blood, and in particular in platelet-rich plasma (PRP) and/or in isolated platelet (IP) [22] as well as in gastric tissue for detection of peptides [12];

**iii) in vivo**, in brain extracellular fluid when the sensor is stereotactically implanted in discrete brain

areas of anesthetized as well as freely moving animals [4,10,23]. In particular, in vivo the DPV methodology associated with carbon fiber micro electrodes (DPV- $\mu$ CFE) becomes an advanced approach to monitoring changes in monoamine release and their metabolism. Indeed, the method fulfills many of the criteria required to monitor specific compounds in the extracellular fluid [5] in brief:

- The undersized probe allows sampling a region of approximately  $10^{-6}$  mm<sup>3</sup> volume i.e. there is high anatomical resolution of the site of measurement within discrete brain areas of rodents, with minimal damage to the nervous tissue.
- The method allows rapid, repeated measurements with accurate time resolution in vivo, in situ in real time without requiring perfusion, sample preparation, chromatographic separation or radio-labeled transmitter supplies. This is the fundamental difference between voltammetry and the perfusion techniques such as micro-dialysis [24, 25].
- The association DPV -  $\mu$ CFE can be performed in vivo in conscious freely moving animals. This solves

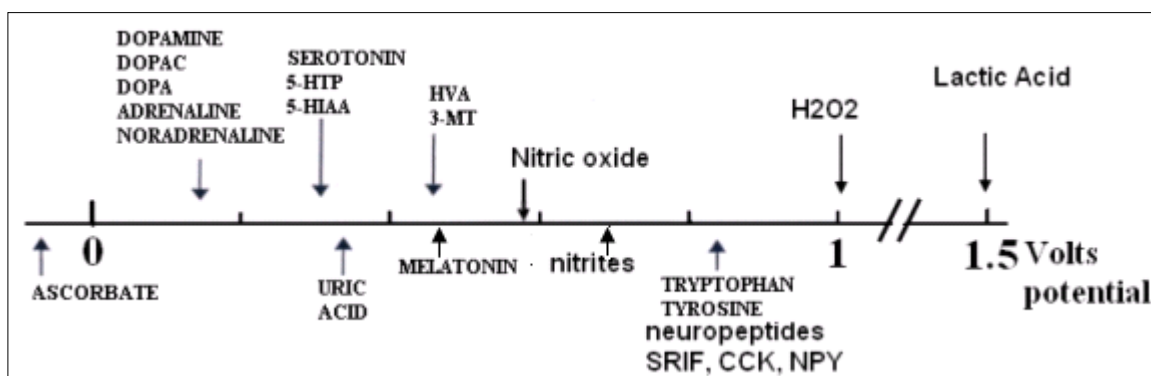


Figure 5. Electro-active compounds measurable at selective oxidation potentials in vitro as well as in vivo with the association DPV -  $\mu$ CFE (modified from ref 5 with permission)..

the problems associated with anesthetics and allows correlations between neuronal activity and behavior [5, 6].

Pharmacological experiments performed with DPV -  $\mu$ CFE have indeed demonstrated that the following chemicals can be selectively monitored in vivo in brain areas:

- Ascorbate, noradrenaline and/or dopamine and the metabolites DOPAC, homovanillic acid, 3-methoxytyramine [26 - 29];
- Uric acid, [30];
- 5-OH-indoles (i.e. serotonin and its metabolite 5-OH-indolacetic acid) [8, 10, 13, 23].

In addition to the detection of monoamine release and their metabolism, in particular those of dopamine and serotonin, other electro-active chemicals have been successively detected with the association DPV -  $\mu$ CFE in vitro as well as in vivo as shown in figure 5. In particular, melatonin [31, 32] nitric oxide and nitrites [21, 33, 34] have been monitored between 500 and 700mV oxidation potential. Furthermore, neuropeptides containing electro-active amino acids such as tryptophan, cysteine, tyrosine appear to be electrochemically active in vitro; their oxidation potentials occur between +600 and +900mV [35 - 37] so that they are well demarcated from the selective DPV voltammetric oxidation peaks linked to the monoamines, the related metabolites and the other compounds mentioned above. Thus, the associated peptidergic oxidation signal has been called Peak

5 and it has been demonstrated that it is linked to the in situ oxidation of somatostatin (SRIF) [35, 37], cholecystokinin (CCK) [38 - 40] or neuropeptide Y (NPY) [41] depending on the discrete brain region analyzed. Hydrogen peroxide (H<sub>2</sub>O<sub>2</sub>) was also successively monitored in vivo, in situ and in real time in rat brain at approximately 1000mV [42].

Variations of the pulse polarography technique have also been proposed. In particular Differential Square Pulse Conditioning Voltammetry has been introduced since it is permitting longer "life" to the micro sensor when used in vivo [43, 44]. Another variant is Short Range Differential Pulse Polarography that couples sensitivity and selectivity with very rapid measurement of endogenous chemicals [45, 46]. Again, Differential Pulse Stripping Voltammetry, characterized by the addition to a DPV scan of a conditioning potential followed by a cleaning potential, permits nearly continuous measurements without loss of sensitivity. This is a clear advantage when one need to combine the analysis of behavior with related changes of neurotransmitters, for instance.

Finally, a very recent achievement of the association DPV -  $\mu$ CFE is the evidence of the feasibility of monitoring Lactic Acid both in vitro and in vivo in the frontal cortex of rodents at the selective oxidation potential +1.5 Volts [47] (see Figure 5).

It appears therefore evident that this electrochemical methodology is still evolving in detecting a variety of chemicals, at the same time as presenting a range of advantages over methods based on the



preparation of samples and/or separation steps. Indeed, it allows rapid, direct, concomitant finding of different chemicals based upon specific oxidative (or red-ox) potentials either in vitro, ex vivo and in vivo conditions [48].

Such a flexibility of application is illustrated by the feasibility to couple this methodology with behavioral observations [49], with electrophysiological recordings, for example of the sleep-awake cycle [23] as well as with in vivo cell firing [36, 50, 51].

A particular example of such flexibility of utilization is the feasibility to apply the methodology in physiologic as well as pathological conditions, thus proposing selective mechanisms of actions of the neurotransmitters that can be monitored in vivo, in situ and in real time. This, taken together with the recent improvement in the methodology permitting DPV voltammetric analysis in telemetric – wireless conditions, thus allowing electrochemical studies in absolutely freely moving conditions [52] may help in the understanding of cerebral diseases and possibly in the development of pharmacological approaches to tackle them [53 – 60].

## References

- Adams, RN. (1969 a) Application of modern electroanalytical techniques to pharmaceutical chemistry. *J. Pharm. Sci.* 58, 1171 -1178
- Adams, RN. (1969 b) Rapid voltage sweep methods at stationary electrodes In *Electrochemistry at Solid Electrodes*. Marcel Dekker, N. Y .
- Shah AJ, Crespi F, Heidbreder C. (2002) Amino acid neurotransmitters: separation approaches and diagnostic value. [Review] *Journal of Chromatography B: Analytical Technologies in the Biomedical & Life Sciences*. 781(1-2),151-163.
- Stamford J, Crespi F, Marsden CA. (1992) In vivo voltammetric methods for monitoring monoamine release and metabolism. In *Practical Approach Series Monitoring Neuronal Activity*. Irl Press at Oxford University Press: Oxford, U.K. pp.113-145.
- Crespi F. (2013) Serotonin, how to find it...Review Article Xjenja Online - Journal of Malta Chamber of Scientists <http://www.mcs.org.mt/> Doi: <http://dx.medra.org/10.7423/XJENZA..2.02, 14-22>.
- Crespi F. (2014) Invasive or Non-Invasive Techniques and Sensors for Real Time In Vivo Sensing in the Brain" chapter in the book, *Laboratory and Clinical Research: "Microelectrodes: Techniques, Structures for Biosensing and Potential Applications"* Nova Biomedical Science Publishers, Inc (Kin Fong Ley ED.) ISBN: 978-1-62948-721-2 (e-book)
- Ponchon JL, Cespuoglio R, Gonon F, Jouvet M, Pujol JF. (1979) Normal pulse polarography with carbon fiber electrodes for in vitro and in vivo determination of catecholamines *Anal. Chem.* 51 (9), 1483-1486. <https://doi.org/10.1021/ac50045a030>.
- Martin KF, Marsden CA, Crespi F. (1988) In vivo electrochemistry with carbon fibre electrodes: principles and application to neuropharmacology. *Trends Anal. Chem.* 7 (9), 334-339.
- Self T, Crespi F. (1992) Electron microscopic and voltammetric analysis of carbon fibre electrode pretreatments. *Journal of Materials in Medicine* 3, 418-425.
- Crespi F. (1990) In vivo voltammetry with micro-biosensors for analysis of neurotransmitter release and metabolism. *Journal of Neuroscience Methods* 34, 53-65.
- Crespi F, Vecchiato E, Lazzarini C, Gaviraghi G. (2001) Electrochemical evidence that lacidipine stimulates release of nitrogen monoxide (NO) in rat aorta. *Neuroscience Letters* 298, 171-174.
- Crespi F. (2017) Central [CNS] and Peripheral [Gastric Tissue] Selective Monitoring of Somatostatin (SRIF) with Micro-Sensor and Voltammetry in Rats: Influence of Growth Factors (GH, EGF). *Biosensors* 7 (4), 53-63. doi:10.3390/bios 7040052
- Crespi F, Martin KF, Marsden CA. (1988) Nafion coated carbon fibre electrodes combined with differential pulse voltammetry measure 5HT release in vivo. *Neuroscience* 27, 885-896
- Baumeyer T, Dittrich J, Crespi F. (1993) Nafion-crown ether modified carbon fibre electrodes: new microbiosensors for detection of neurotransmitters in vitro and in vivo. *Electroanalysis* 5 (7), 565-570.
- Mobius M, Crespi F. (1992) In vivo selective

- monitoring of basal levels of cerebral dopamine using voltammetry with NAFION-CROWN ETHER carbon fibre microsensors. *Journal of Neuroscience Methods* 42, 149-161.
16. Flato JB. (1972) The renaissance in polarographic and voltammetric analysis. *Analyt. Chem.* 44, 78-87.
  17. Goutier W, Lowry JP, McCreary AC, et al. (2016) Frequency-Dependent Modulation of Dopamine Release by Nicotine and Dopamine D1 Receptor Ligands: An In Vitro Fast Cyclic Voltammetry Study in Rat Striatum. *Neurochem Res* 41, 945-950. <https://doi.org/10.1007/s11064-015-1786-8>
  18. Bull D, Palij M, Millar J, et al. (1990) Application of fast cyclic voltammetry to measurement of electrically evoked dopamine overflow from brain slices in vitro. *J. Neurosci. Methods* 32, 37-44.
  19. Rice ME, Patel JC, Cragg SJ. (2011) Dopamine release in the basal ganglia. *Neuroscience* 198, 112-137. <https://doi.org/10.1016/j.neuroscience.2011.08.066>
  20. Cristofori P, Crivellente F, Faustinelli I, Turton J, Zancanaro C, Crespi F. (2004) Involvement of the NITROGEN MONOXIDE (NO) system in the anti-atherosclerotic potential of LACIDIPINE in Apo-E deficient mouse: A morphological, functional and electrochemical study. *Toxicologic Pathology* 32, 493-499.
  21. Rossetti Z, Crespi F. (2004) Inhibition of Nitric Oxide release in vivo by ethanol Alcoholism: Clinical and Experimental Research 28, 1-6.
  22. Bianchi M, Moser C, Lazzarini C, Vecchiato E, Crespi F. (2002) Forced swimming test and fluoxetine treatment: in vivo evidence that Periphil 5-HT in rat platelet-rich plasma mirrors cerebral extracellular 5-HT levels, whilst 5-HT in isolated platelets mirrors neuronal 5-HT changes. *Experimental Brain Research* 143, 191-197.
  23. Crespi F, Jouvét M. (1983) Differential pulse voltammetry: parallel peak 3 changes with vigilance states in raphe dorsalis and raphe magnus of chronic freely moving rats and evidence for 5HT contribution to this peak after monoamine oxidase inhibitors. *Brain Research* 272, 263-268.
  24. Ungerstedt U, Hallström A. (1987) In vivo microdialysis - a new approach to the analysis of neurotransmitters in the brain *Life Sciences* 41 (7), 861-864 [https://doi.org/10.1016/0024-3205\(87\)90181-0](https://doi.org/10.1016/0024-3205(87)90181-0)
  25. Ortega JE, Meana JJ, Callado LF. (2016) In Vivo Brain Microdialysis of Monoamines. In: Luján R., Ciruela F. (eds) *Receptor and Ion Channel Detection in the Brain. Neuromethods*, vol 110. Humana Press, New York, NY
  26. Buda M, Gonon F, Cespuoglio R, Jouvét M, Pujol JF. (1981) In vivo electrochemical detection of catechols in several dopaminergic brain regions of anaesthetized rats. *European Journal of Pharmacology* 73 (1), 61-68. [https://doi.org/10.1016/0014-2999\(81\)90145-X](https://doi.org/10.1016/0014-2999(81)90145-X)
  27. Crespi F, Keane P. (1987) Analysis of extracellular DOPAC, HVA, 5-HIAA and ascorbic acid in rat striatum in vivo by DPV, effect of PCP, haloperidol and their co-administration. *Research Communications* 19, 639-649.
  28. Crespi F, Martin KF, Heal DJ, Marsden CA, Buckett WR, Sanghera MK. (1989) Measurement of 3 methoxytyramine by in vivo voltammetry: evidence for differences in cerebral dopamine function in Balb/c and CBA mice. *Brain Research* 500, 241-246.
  29. Sanghera M, Crespi F, Martin K, Heal DJ, Buckett WR, Marsden CA. (1990) Biochemical and in vivo voltammetric evidence for difference in striatal dopamine levels in inbred strains of mice. *Neuroscience* 39 (3), 649-656.
  30. Crespi F, Sharp T, Maidment N, Marsden CA. (1983) Differential pulse voltammetry in vivo, evidence that the uric acid contributes to the indole oxidation peak. *Neuroscience Letters* 43, 203-207.
  31. Crespi F, Ratti E, Trist DG. (1994) Melatonin, a hormone monitorable in vivo by voltammetry? *The Analyst* 119, 2193-2197
  32. Crespi F. (2012) Influence of melatonin or its antagonism on alcohol consumption in ethanol drinking rats: a behavioural and in vivo voltammetric study. *Brain Research* 1452, 39-46.
  33. Crespi F, Campagnola M, Neudeck A, McMillan K, et al. (2001) Can voltammetry measures nitrogen monoxide (NO) and/or nitrites? *Journal of*

- Neuroscience Methods 109, 59-70.
34. Crespi F. (2013) In vivo voltammetric evidence that cerebral nitric oxide (NO) is influenced by drugs of abuse: Is NO implicated in their neurotoxicity? RSC Adv.3, 9803–9808. This journal is @ The Royal Society of Chemistry
  35. Crespi F. (1991) In vivo voltammetry detection of neuropeptides with micro carbon fibre biosensors: possible selective detection of somatostatin. Analytical Biochemistry 194, 1-8.
  36. Crespi F. (2002) In vivo voltammetry and concomitant electrophysiology at a single biosensor to analyse ischaemia, depression and drug dependence. Journal of Neuroscience Methods 119, 173-184.
  37. Crespi F. (2017) Central [CNS] and Peripheral [Gastric Tissue] Selective Monitoring of Somatostatin (SRIF) with Micro-Sensor and Voltammetry in Rats: Influence of Growth Factors (GH, EGF). Biosensors 7(4), 53-63. doi:10.3390/bios 7040052
  38. Crespi F. (1998) The role of cholecystokinin (CCK), CCK-A or CCK-B receptor antagonists in the spontaneous preference for drugs of abuse (alcohol or cocaine) in naive rats. Methods Find Exp Clin Pharmacol 20 (8), 679-97.
  39. Crespi F, Corsi M, Reggiani A, Ratti E, Gaviraghi G. (2000) Involvement of cholecystokinin within craving for cocaine: role of cholecystokinin receptor ligands Expert Opin Investig Drugs 9(10),2249-2258.
  40. Crespi F, Congestri F, Formenti F. (2019) Evidence that ethanol selectively alters dopamine and serotonin metabolism as well as peptidergic levels in CA3 hippocampus of spontaneously alcohol preferring rats. Clin Res Trials 5: doi: 10.15761/CRT.1000247
  41. Crespi F. (2011) Influence of Neuropeptide Y and antidepressants upon cerebral monoamines involved in depression: An in vivo electrochemical study. Brain Research 1407, 27-37.
  42. Crespi F. (2014) Hydrogen peroxide monitored in vivo, in situ and in real time in rat brain, is it a marker of central cholinergic dynamics? Analytical Methods, 6, 1174–1181 DOI: 10.1039/c3ay41682h
  43. Baumeier T, Dittrich J, Crespi F. (1990) Differential square pulse conditioning voltammetry: a new method for electrochemical analysis with micro-biosensors. British Journal of Pharmacology 99, 260.
  44. Crespi F, Baumeier T, Dittrich J. Simultaneous in vivo monitoring of dopamine and serotonin by differential pulse conditioning voltammetry with Na-cro microbiosensors. Fresenius Journal of Analytical Chemistry 341 (10), 644.
  45. Neudeck A. Crespi F. (1992) Short Range Differential Pulse Polarography for fast, selective analysis of cerebral electroactive compounds in vivo. British Journal of Pharmacology 107, 427.
  46. Crespi F, Neudeck A. (1993) Short Range Differential Pulse Voltammetry for fast, selective analysis of basal levels of cerebral compounds in vivo. Journal of Neuroscience Methods 50, 225-235
  47. Crespi F. (2019) Feasibility analysis of lactic acid detection by in vivo voltammetry in the rat brain: Influence of oxygen and carbon dioxide. Current Topics in Analytical Chemistry 11, 51-58.
  48. Sanghavi BJ, Wolfbeis OS, Hirsch T, Swam, NS. (2015) Nanomaterial-based electrochemical sensing of neurological drugs and neurotransmitters. Mikrochim. Acta 182, 1–41.
  49. Crespi F. (2010) Is a divergent central serotonergic activity responsible for either despair or learning behavior in intact Wistar or Sprague-Dawley CD rats, respectively? A concomitant behavioral and electrochemical analysis. PSYCHOLOGY 1, 1-11.
  50. Formenti, F., Sonntag V., Congestri F., Crespi F. (2009) Dopamine D3 Receptor Antagonist SB-277011A Influences Cell Firing in the Rat VTA, Parallel Role with the Cannabinoid System in Addiction and Neuropsychiatry Disorders? The Open Neuropsychopharmacology Journal, 2, 86-92.
  51. Crespi F. (2009) Anxiolytics antagonize Yohimbine-induced central noradrenergic activity: a concomitant in vivo voltammetry – electrophysiology model of anxiety. Journal of Neuroscience Methods 180, 97-105.
  52. Crespi F. (2010) Wireless in vivo voltammetric



- measurements of neurotransmitters in freely behaving rats. *Biosensors and Bioelectronics* 25, 2425–2430.
53. Crespi F, Jouvet M. (1982) Sleep and indolamine alterations induced by thiamine deficiency. *Brain Research* 248, 275-283.
54. Crespi F. (1986) Influence of stress and of stress-related peptides on the cerebral metabolism of dopamine and serotonin measured in the striatum of conscious freely moving rats. *Medicina Riv E.M.I.* 6, 379-382.
55. Crespi F. (1989) Influence of forced immobilisation and of stress-related peptides on striatal DOPAC and 5HIAA voltammetrically detected in freely moving rats. *Regulatory Peptides* 26 (1) 65.
56. Crespi F, Mobius M, Wright IK. (1992) Isolation rearing of rats alters behaviour and release of 5-hydroxytryptamine and dopamine in the frontal cortex. *Experimental Brain Research* 88, 495-501.
57. Crespi F. (1996) Concomitant in vivo electrophysiological and voltammetric analysis indicate that ascorbic acid is a biochemical index of early ischaemia. *Neuroscience Letters* 215, 189-192.
58. Crespi F, Pietra C. (1997) Middle cerebral artery occlusion alters neurotransmitter activities in ipsilateral and contralateral rat brain regions: an ex vivo voltammetric study. *Neuroscience Letters* 230, 77-80.
59. Crespi F, Bianchi M. (2002) Serotonin and neuronal plasticity relationship: a new mechanism involved in depression? *European Neuropsychopharmacology* 12, 191.
60. Crespi F. (2019) Concomitant in vivo voltammetric and electrophysiological analysis indicate that nociceptin/orphanin FQ may affect dopamine and then serotonin activities in the substantia nigra. *Int. Physiol. J.* 2 (3), 1-9. DOI: 10.14302/issn25-78-8590.ipj-19-2772.